

QuantiTect® Probe RT-PCR Handbook

For quantitative, real-time one-step RT-PCR
using sequence-specific probes



QIAGEN Sample and Assay Technologies

QIAGEN is the leading provider of innovative sample and assay technologies, enabling the isolation and detection of contents of any biological sample. Our advanced, high-quality products and services ensure success from sample to result.

QIAGEN sets standards in:

- Purification of DNA, RNA, and proteins
- Nucleic acid and protein assays
- microRNA research and RNAi
- Automation of sample and assay technologies

Our mission is to enable you to achieve outstanding success and breakthroughs. For more information, visit www.qiagen.com.

Contents

Kit Contents	4
Shipping and Storage	4
Product Use Limitations	4
Product Warranty and Satisfaction Guarantee	5
Technical Assistance	5
Safety Information	5
Product Description	6
Quality Control	7
Introduction	8
One-step RT-PCR	8
Use of uracil-N-glycosylase (UNG)	10
Sequence-specific probes	10
Using the correct protocol	12
Protocols	
■ Real-Time One-Step RT-PCR Using Applied Biosystems Cyclers and Other Cyclers	13
■ Real-Time One-Step RT-PCR Using the LightCycler 1.x and 2.0	16
Troubleshooting Guide	20
Ordering Information	26

Kit Contents

QuantiTect Probe RT-PCR Kit	(200)	(1000)
Catalog no.	204443	204445
Number of 50 µl reactions	200	1000
2x QuantiTect Probe RT-PCR Master Mix, containing:	3 x 1.7 ml	25 ml
■ HotStarTaq® DNA Polymerase		
■ QuantiTect Probe RT-PCR Buffer		
■ dNTP mix, including dUTP		
■ ROX™ passive reference dye		
■ 8 mM MgCl ₂		
QuantiTect RT Mix, a mixture of the QIAGEN® products:	100 µl	500 µl
■ Omniscript® Reverse Transcriptase		
■ Sensiscript® Reverse Transcriptase		
RNase-Free Water	2 x 2 ml	20 ml
Handbook	1	1

Shipping and Storage

The QuantiTect Probe RT-PCR Kit is shipped on dry ice. The kit should be stored immediately upon receipt at –20°C in a constant-temperature freezer and protected from light. When the kit is stored under these conditions and handled correctly, performance is guaranteed until the expiration date (see the quality-control label inside the kit box or on the kit envelope). 2x QuantiTect Probe RT-PCR Master Mix can also be stored protected from light at 2–8°C for up to 6 months, depending on the expiration date, without showing any reduction in performance. However, QuantiTect RT Mix must always be stored at –20°C to guarantee performance.

To maintain optimal performance of the QuantiTect Probe RT-PCR Kit for 1000 x 25 µl reactions, we recommend storing the 25 ml master mix as appropriately sized aliquots in sterile, polypropylene tubes.

Product Use Limitations

The QuantiTect Probe RT-PCR Kit is intended for molecular biology applications. This product is not intended for the diagnosis, prevention, or treatment of disease.

All due care and attention should be exercised in the handling of the products. We recommend all users of QIAGEN products to adhere to the NIH guidelines that have been developed for recombinant DNA experiments, or to other applicable guidelines.

Product Warranty and Satisfaction Guarantee

QIAGEN guarantees the performance of all products in the manner described in our product literature. The purchaser must determine the suitability of the product for its particular use. Should any product fail to perform satisfactorily due to any reason other than misuse, QIAGEN will replace it free of charge or refund the purchase price. We reserve the right to change, alter, or modify any product to enhance its performance and design. If a QIAGEN product does not meet your expectations, simply call your local Technical Service Department or distributor. We will credit your account or exchange the product — as you wish. Separate conditions apply to QIAGEN scientific instruments, service products, and to products shipped on dry ice. Please inquire for more information.

A copy of QIAGEN terms and conditions can be obtained on request, and is also provided on the back of our invoices. If you have questions about product specifications or performance, please call QIAGEN Technical Services or your local distributor (see back cover or visit www.qiagen.com).

Technical Assistance

At QIAGEN, we pride ourselves on the quality and availability of our technical support. Our Technical Service Departments are staffed by experienced scientists with extensive practical and theoretical expertise in sample and assay technologies and the use of QIAGEN products. If you have any questions or experience any difficulties regarding the QuantiTect Probe RT-PCR Kit or QIAGEN products in general, please do not hesitate to contact us.

QIAGEN customers are a major source of information regarding advanced or specialized uses of our products. This information is helpful to other scientists as well as to the researchers at QIAGEN. We therefore encourage you to contact us if you have any suggestions about product performance or new applications and techniques.

For technical assistance and more information, please see our Technical Support Center at www.qiagen.com/Support or call one of the QIAGEN Technical Service Departments or local distributors (see back cover or visit www.qiagen.com).

Safety Information

When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, please consult the appropriate material safety data sheets (MSDSs). These are available online in convenient and compact PDF format at www.qiagen.com/Support/MSDS.aspx where you can find, view, and print the MSDS for each QIAGEN kit and kit component.

24-hour emergency information

Emergency medical information in English, French, and German can be obtained 24 hours a day from:

Poison Information Center Mainz, Germany

Tel: +49-6131-19240

Product Description

Component	Description
HotStarTaq DNA Polymerase*	HotStarTaq DNA Polymerase is a modified form of a recombinant 94 kDa DNA polymerase, originally isolated from <i>Thermus aquaticus</i> , cloned into <i>E. coli</i> . (Deoxynucleoside-triphosphate: DNA deoxynucleotidyltransferase, EC 2.7.7.7).
QuantiTect Probe RT-PCR Buffer*	Contains Tris-Cl, KCl, $(\text{NH}_4)_2\text{SO}_4$, 8 mM MgCl_2 , pH 8.7 (20°C)
dNTP mix*	Contains dATP, dCTP, dGTP, and dUTP of ultrapure quality
Fluorescent dyes*	ROX
QuantiTect RT Mix	Contains an optimized mixture of the QIAGEN products Omniscript Reverse Transcriptase and Sensiscript Reverse Transcriptase, both of which are recombinant heterodimeric enzymes expressed in <i>E. coli</i> .
RNase-free water	Ultrapure quality, PCR-grade

* Included in 2x QuantiTect Probe RT-PCR Master Mix.

Quality Control

Component	Test
QuantiTect Probe RT-PCR Master Mix*	RT-PCR sensitivity and reproducibility assay: Sensitivity and reproducibility in real-time RT-PCR are tested in parallel 50 µl reactions containing 10-fold dilutions of nucleic acid template.
HotStarTaq DNA Polymerase†	Efficiency and reproducibility in PCR are tested. Functional absence of exonucleases and endonucleases is tested.
QuantiTect Probe RT-PCR Buffer†	Conductivity and pH are tested.
QuantiTect RT Mix	Efficiency of cDNA synthesis and functional absence of RNases, exonucleases, and endonucleases are tested.
RNase-free water	Conductivity, pH, and RNase activities are tested.

* See quality-control label inside the kit box or on the kit envelope for lot-specific values.

† Included in 2x QuantiTect Probe RT-PCR Master Mix.

Introduction

The QuantiTect Probe RT-PCR Kit provides accurate real-time quantification of RNA targets in an easy-to-handle format. The kit is designed for use with all types of probe, including TaqMan® dual-labeled probes, FRET probes, and Molecular Beacons. High specificity and sensitivity in RT-PCR are achieved by the use of the hot-start enzyme HotStarTaq DNA Polymerase together with a specialized RT-PCR buffer. The buffer also contains ROX dye, which allows fluorescence normalization on certain cyclers. The optimized Omniscript and Sensiscript blend for the reverse-transcription step further enhances sensitivity.

The kit has been optimized for use with any real-time cycler, including Rotor-Gene® cyclers* and instruments from Applied Biosystems®, Bio-Rad, Cepheid, Eppendorf, Roche, and Agilent (formerly Stratagene). This handbook contains general protocols for use with cyclers from these suppliers.

One-step RT-PCR

Use of 2x QuantiTect Probe RT-PCR Master Mix together with QuantiTect RT Mix allows both reverse transcription and PCR to take place in a single tube. All reagents required for both reactions are added at the beginning, so there is no need to open the tube once the reverse-transcription reaction has been started.

The components of 2x QuantiTect Probe RT-PCR Master Mix include HotStarTaq DNA Polymerase, QuantiTect Probe RT-PCR Buffer, and ROX passive reference dye (see descriptions below). QuantiTect RT Mix contains an Omniscript and Sensiscript blend (see descriptions below).

Omniscript and Sensiscript Reverse

QuantiTect RT Mix contains an optimized Omniscript and Sensiscript blend. Both enzymes exhibit a high affinity for RNA, facilitating transcription through secondary structures that may inhibit other reverse transcriptases. Omniscript is designed for reverse transcription of RNA amounts greater than 50 ng, and Sensiscript is optimized for use with very small amounts of RNA (<50 ng). This enzyme combination provides highly efficient and sensitive reverse transcription over a wide range of RNA template amounts.

* To take advantage of the fast-cycling capabilities of Rotor-Gene cyclers, use optimized Rotor-Gene Kits; for details, visit www.qiagen.com/goto/Rotor-GeneKits.

HotStarTaq DNA Polymerase

HotStarTaq DNA Polymerase is a modified form of QIAGEN *Taq* DNA Polymerase, and is provided in an inactive state and has no enzymatic activity at ambient temperature. The enzyme remains completely inactive during the reverse-transcription reaction and does not interfere with it. This prevents formation of misprimed RT-PCR products and primer–dimers during reaction setup, reverse transcription, and the first denaturation step. The enzyme is activated after the reverse-transcription step by a 15-minute, 95°C incubation step. The hot start also inactivates the reverse-transcription enzymes, ensuring temporal separation of reverse transcription and PCR, and allowing both steps to be performed sequentially in a single tube.

QuantiTect Probe RT-PCR Buffer

QuantiTect Probe RT-PCR Buffer is designed to facilitate both efficient reverse transcription and specific amplification in a one-tube format. It is based on the unique QIAGEN OneStep RT-PCR buffer system, and has been specifically adapted for real-time RT-PCR using sequence-specific probes. The buffer contains a balanced combination of KCl and $(\text{NH}_4)_2\text{SO}_4$, which promotes a high ratio of specific to nonspecific primer binding during the annealing step of each PCR cycle. This creates stringent primer annealing conditions, leading to increased PCR specificity. When using this buffer, primer annealing is only marginally influenced by the MgCl_2 concentration, so optimization by titration of Mg^{2+} is usually not required.

Passive reference dye

For certain real-time cyclers, the presence of ROX passive reference dye in real-time PCR compensates for non-PCR-related variations in fluorescence detection. Fluorescence from ROX dye does not change during the course of real-time PCR, but provides a stable baseline to which PCR-related fluorescent signals are normalized. Thus, ROX dye compensates for differences in fluorescence detection between wells due to slight variations in reaction volume or to differences in well position.

The use of ROX dye is necessary for all instruments from Applied Biosystems and is optional for instruments from Agilent (e.g., Mx3000P®, Mx3005P®, and Mx4000®). Rotor-Gene cyclers and instruments from Bio-Rad, Cepheid, Eppendorf, and Roche do not require ROX dye. The presence of ROX dye in the master mix does not interfere with real-time PCR on any instrument, since the dye is not involved in the reaction and has an emission spectrum completely different from fluorescent dyes commonly used for probes.

Use of uracil-N-glycosylase (UNG)

The QuantiTect Probe RT-PCR Kit contains dUTP, which replaces dTTP. The QuantiTect Probe RT-PCR Kit therefore allows the optional use of a uracil-N-glycosylase (UNG) pretreatment of the reaction if contamination with carried-over PCR products is suspected.

However, only **heat-labile** UNG can be used, since UNG isolated from *E. coli* is stable at elevated temperatures and will destroy any cDNA synthesized during the RT step at 50°C. Heat-labile UNG is active only at the very beginning of the RT step and will eliminate any dUMP-containing RT-PCR products resulting from carryover contamination. After a few minutes, the heat-labile UNG will have lost any activity and therefore cannot interfere with cDNA synthesis.

Note: UNG is not included in the QuantiTect Probe RT-PCR Kit and must be purchased separately.

Sequence-specific probes

The QuantiTect Probe RT-PCR Kit can be used with all types of probe. The 2 major types of sequence-specific probe used for real-time PCR are described briefly below. For a more detailed description of these probes and their design and for other probe types not mentioned here, see "Guidelines for real-time PCR" at www.qiagen.com/resources/info.

Dual-labeled probes

Dual-labeled probes, including TaqMan probes, are sequence-specific oligonucleotides with a fluorophore and a quencher moiety attached (Figure 1). The fluorophore is at the 5' end of the probe, and the quencher moiety is usually located at the 3' end or internally. During the extension phase of PCR, the probe is cleaved by the 5'→3' exonuclease activity of *Taq* DNA Polymerase, separating the fluorophore and the quencher moiety. This results in detectable fluorescence that is proportional to the amount of accumulated PCR product.

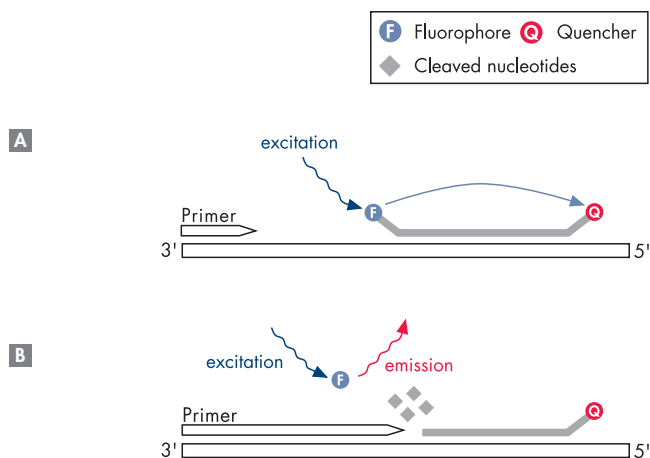


Figure 1. Schematic diagram of the principle of dual-labeled probes in quantitative, real-time PCR. **A** Both the dual-labeled probe and the PCR primers anneal to the target sequence during the PCR annealing step. The proximity of the fluorophore with the quencher prevents the fluorophore from fluorescing. **B** During the PCR extension step, *Taq* DNA Polymerase extends the primer. When the enzyme reaches the dual-labeled probe, its 5'→3' exonuclease activity cleaves the fluorophore from the probe. The fluorescent signal from the free fluorophore is measured.

FRET probes

Real-time PCR with fluorescence resonance energy transfer (FRET) probes, such as LightCycler® hybridization probes, uses 2 labeled oligonucleotide probes that bind to the PCR product in a head-to-tail fashion (Figure 2). When the 2 probes bind, their fluorophores come into close proximity, allowing energy transfer from a donor fluorophore to an acceptor fluorophore. This causes fluorescence that is proportional to the amount of PCR product. FRET probes are not cleaved during the reaction, and can bind to a target again in the next PCR cycle.

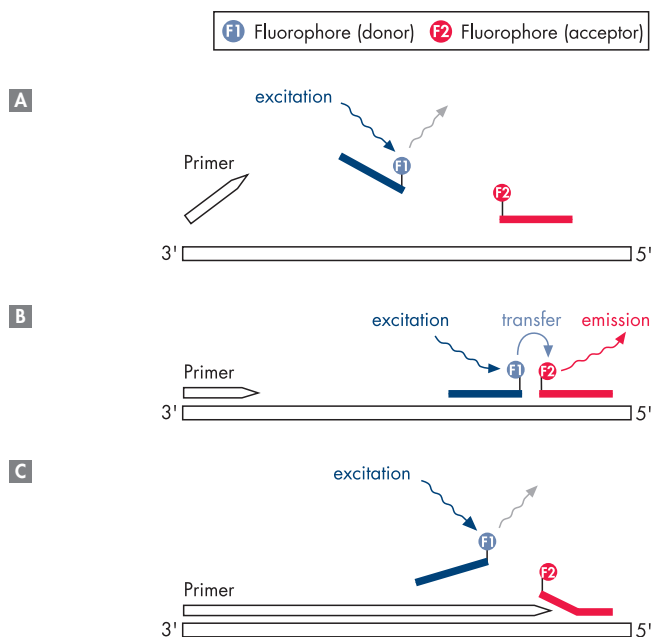


Figure 2. Principle of FRET probes in quantitative, real-time PCR. **A** When the FRET probes are not bound to the target sequence, no fluorescent signal from the acceptor fluorophore is detected. **B** During the PCR annealing step, both FRET probes hybridize to the target sequence. This brings the donor fluorophore and acceptor fluorophore into close proximity, allowing energy transfer between the fluorophores and resulting in a fluorescent signal from the acceptor fluorophore that is measured. The amount of signal is proportional to the amount of target sequence, allowing quantification of the amount of target sequence. **C** During the PCR extension step, the FRET probes are displaced from the target sequence and the acceptor fluorophore is no longer able to generate a fluorescent signal.

Using the correct protocol

This handbook contains 2 protocols. The first protocol (page 13) is for use with most real-time cyclers, including Rotor-Gene cyclers and instruments from Applied Biosystems, Bio-Rad, Cepheid, Eppendorf, Roche, and Agilent. The second protocol (page 16) is for use with the LightCycler 1.x and LightCycler 2.0 only.

For background information on real-time PCR, please refer to “Guidelines for real-time PCR” at www.qiagen.com/resources/info, which contains guidelines on template preparation, primer and probe design, controls, data analysis, and other topics.

Protocol: Real-Time One-Step RT-PCR Using Applied Biosystems® Cyclers and Other Cyclers

This protocol is intended for use with dual-labeled probes (e.g., TaqMan) and most real-time cyclers, including Rotor-Gene cyclers and instruments from Applied Biosystems, Bio-Rad, Cepheid, Eppendorf, Roche, and Agilent. If using the **LightCycler 1.x** or **LightCycler 2.0**, follow the protocol on page 16.

Reaction volume

A reaction volume of 50 µl should be used with most real-time cyclers. However, the reaction volume must be reduced to 25 µl if using the **Applied Biosystems 7500 Fast System** or a **SmartCycler® system**, or to 10 µl if using a **LightCycler 480**.

When reducing the reaction volume, remember to reduce the volume of master mix and RT mix used in the reaction: the volume of 2x QuantiTect Probe RT-PCR Master Mix should always be half of the final reaction volume, and the volume of QuantiTect RT Mix should always be one-hundredth of the final reaction volume. In addition, be sure to keep the concentration of primers, probe, template, and UNG the same as described in Table 1.

Important points before starting

- Always start with the cycling conditions specified in this protocol, even if using previously established primer–probe systems.
- For the highest efficiency in real-time RT-PCR using sequence-specific probes, targets should ideally be **100–150 bp in length**.
- After reverse transcription, the PCR step of the RT-PCR must start with an **initial incubation step of 15 min at 95°C** to activate HotStarTaq DNA Polymerase.
- Set up all reactions on ice to avoid premature cDNA synthesis.
- The kit has been optimized for a final reaction volume of 50 µl. If other reaction volumes are used, adjust the amounts of 2x QuantiTect Probe RT-PCR Master Mix and QuantiTect RT Mix used so that the ratio between them remains constant.
- Always readjust the threshold value for analysis of every run.
- 2x QuantiTect Probe RT-PCR Master Mix contains dUTP, which allows the use of a uracil-N-glycosylase (UNG) pretreatment of the reaction. Only **heat-labile** UNG should be used.
- If using the **Applied Biosystems 7500**, it is necessary to adjust the preset threshold value to a lower value. Use a value of 0.01 as a starting point.

Procedure

1. Thaw 2x QuantiTect Probe RT-PCR Master Mix (if stored at -20°C), template RNA, primer and probe solutions, and RNase-free water. Mix the individual solutions, and place them on ice. QuantiTect RT Mix should be taken from -20°C immediately before use, always kept on ice, and returned to storage at -20°C immediately after use.
2. Prepare a reaction mix according to Table 1.

Keep samples on ice while preparing the reaction mix.

If final reaction volumes other than 50 μl are used, adjust the volumes of 2x QuantiTect Probe RT-PCR Mix and QuantiTect RT Mix used so that the ratio between them remains constant.

Note: We strongly recommend starting with an initial Mg^{2+} concentration of 4 mM as provided by 2x QuantiTect Probe RT-PCR Master Mix. For a few targets, reactions may be improved by using Mg^{2+} concentrations of up to 6 mM.

Table 1. Reaction setup

Component	Volume/reaction	Final concentration
2x QuantiTect Probe RT-PCR Master Mix*	25 μl [†]	1x
Primer A	Variable	0.4 μM [‡]
Primer B	Variable	0.4 μM [‡]
Probe	Variable	0.1–0.2 μM [§]
QuantiTect RT Mix	0.5 μl [¶]	
Template RNA (added at step 4)	Variable	1 pg to 500 ng/ reaction
RNase-free water	Variable	
Optional: Uracil-N-glycosylase, heat-labile	Variable	2 units/reaction
Total reaction volume	50 μl	

* Provides a final concentration of 4 mM MgCl_2 .

[†] If using a total reaction volume other than 50 μl , calculate the volume of 2x master mix required using this formula: Volume of 2x master mix (μl) = $0.5 \times [\text{Total reaction volume } (\mu\text{l})]$

[‡] A final primer concentration of 0.4 μM is optimal for most applications. However, for individual determination of optimal primer concentration, a primer titration from 0.4 μM to 1 μM can be performed. SmartCycler users should use a final primer concentration of 1 μM for each primer; if necessary, a primer titration from 0.5 μM to 2 μM can be performed to determine the optimal primer concentration.

[§] SmartCycler users should use a final probe concentration of 0.2 μM .

[¶] If using a total reaction volume other than 50 μl , calculate the volume of RT mix required using this formula: Volume of RT mix (μl) = $0.01 \times [\text{Total reaction volume } (\mu\text{l})]$

3. **Mix the reaction mix thoroughly, and dispense appropriate volumes into PCR tubes or plates.**
Keep the PCR tubes or plates on ice.
4. **Add template RNA (1 pg to 500 ng/reaction) to the individual PCR tubes or wells containing the reaction mix.**
5. **Program your real-time cyclor according to the program outlined in Table 2.**
For optional UNG treatment, leave the samples for at least 5 min on ice.
6. **Place the PCR tubes or plates in the real-time cyclor, and start the cycling program.**

Table 2. Real-time cyclor conditions

Step	Time	Temperature	Additional comments
Reverse transcription	30 min	50°C	Temperatures up to 55°C can be used to eliminate secondary structure in the template RNA
PCR initial activation step	15 min	95°C	HotStarTaq DNA Polymerase is activated by this heating step
2-step cycling:			
Denaturation*	15 s	94°C	
Combined annealing/ extension	60 s	60°C	Perform fluorescence data collection
Number of cycles	40–45		The number of cycles depends on the amount of template RNA and transcript abundance

* SmartCycler users can reduce denaturation time to 1 s to take advantage of cycling capacities.

Protocol: Real-Time One-Step RT-PCR Using the LightCycler 1.x and 2.0

This protocol is intended for use with the LightCycler 1.x and LightCycler 2.0 only, and is suitable for FRET probes and dual-labeled probes (e.g., TaqMan). For all other cyclers, follow the protocol on page 13.

Important points before starting

- Always start with the cycling conditions specified in this protocol, even if using previously established primer–probe systems.
- For the highest efficiency in real-time RT-PCR using sequence-specific probes, targets should ideally be **100–150 bp in length**.
- After reverse transcription, the PCR step of the RT-PCR must start with an **initial incubation step of 15 min at 95°C** to activate HotStarTaq DNA Polymerase.
- Set up all reactions in cooled capillaries to avoid premature cDNA synthesis.
- The kit has been optimized for a final reaction volume of 20 µl. If other reaction volumes are used, adjust the amounts of 2x QuantiTect Probe RT-PCR Master Mix and QuantiTect RT Mix used so that the ratio between them remains constant.
- We recommend using the “second derivative maximum” method for data analysis.
- Always readjust the noise band for analysis of every run if using the “fit-point” method for data analysis.
- 2x QuantiTect Probe RT-PCR Master Mix contains dUTP, which allows the use of a uracil-N-glycosylase (UNG) pretreatment of the reaction. Only **heat-labile** UNG should be used.

Procedure

1. **Thaw 2x QuantiTect Probe RT-PCR Master Mix (if stored at –20°C), template RNA, primer and probe solutions, and RNase-free water. Mix the individual solutions, and place them on ice. QuantiTect RT Mix should be taken from –20°C immediately before use, always kept on ice, and returned to storage at –20°C immediately after use.**

2. **Prepare a reaction mix according to Table 3.**

Keep capillaries cooled while preparing the reaction mix.

If final reaction volumes other than 20 µl are used, adjust the volumes of 2x QuantiTect Probe RT-PCR Master Mix and QuantiTect RT Mix used so that the ratio between them remains constant.

Note: We strongly recommend starting with an initial Mg^{2+} concentration of 4 mM as provided by 2x QuantiTect Probe RT-PCR Master Mix. For a few targets, reactions may be improved by using Mg^{2+} concentrations of up to 6 mM.

Table 3. Reaction setup

Component	Volume/reaction	Final concentration
2x QuantiTect Probe RT-PCR Master Mix*	10 μ l	1x
Primer A	Variable	1 μ M [†]
Primer B	Variable	1 μ M [†]
Probe	Variable	0.2 μ M
QuantiTect RT Mix	0.2 μ l	
Template RNA (added at step 4)	Variable	1 pg to 1 μ g/reaction
RNase-free water	Variable	
Optional: Uracil-N-glycosylase, heat-labile	Variable	2 units/reaction
Total reaction volume	20 μl	

* Provides a final concentration of 4 mM $MgCl_2$.

[†] A final primer concentration of 1 μ M is optimal for most applications. However, for individual determination of optimal primer concentration, a primer titration from 0.5 μ M to 2 μ M can be performed.

3. Mix the reaction mix thoroughly, and dispense appropriate volumes into PCR capillaries.

Keep the PCR capillaries cooled.

4. Add template RNA (1 pg to 1 μ g/reaction) to the individual PCR capillaries containing the reaction mix.

For optional UNG treatment, leave the samples for at least 5 min in the cooled capillaries.

5. Program the LightCycler according to the program outlined in Table 4 (FRET probes) or Table 5 (TaqMan and other dual-labeled probes). Set the channels according to Table 6.

6. Place the PCR capillaries in the LightCycler, and start the cycling program.

Table 4. Real-time cyler conditions for FRET probes

Step	Time	Temperature	Ramp rate	Additional comments
Reverse transcription	20 min	50°C	20°C/s	Temperatures up to 55°C can be used to eliminate secondary structures in the template RNA
PCR initial activation step	15 min	95°C	20°C/s	HotStarTaq DNA Polymerase is activated by this heating step
3-step cycling:				
Denaturation	0 s	95°C	20°C/s	
Annealing	30 s	50–60°C	20°C/s	Approximately 5–8°C below T_m of primers. Perform fluorescence data collection.
Extension	30 s	72°C	2°C/s	
Number of cycles	35–55			The number of cycles depends on the amount of template RNA and transcript abundance

Table 5. Real-time cycler conditions for TaqMan and other dual-labeled probes

Step	Time	Temperature	Ramp rate	Additional comments
Reverse transcription	20 min	50°C	20°C/s	Temperatures up to 55°C can be used to eliminate secondary structures in the template RNA
PCR initial activation step	15 min	95°C	20°C/s	HotStarTaq DNA Polymerase is activated by this heating step
2-step cycling:				
Denaturation	0 s	95°C	20°C/s	
Combined annealing/ extension	60 s	60°C	20°C/s	Perform fluorescence data collection
Number of cycles	35–55			The number of cycles depends on the amount of template RNA and transcript abundance

Table 6. Channel settings during run (Display Mode) and for data analysis

	Detection channel	Display mode	Channel settings for data analysis
Dual-labeled probes (FAM™)	F1	F1/1	F1/F2
Hybridization probe (LC®-Red 640)	F2	F2/1	F2/F1
Hybridization probe (LC-Red 705)	F3	F3/1	F3/F1

Troubleshooting Guide

This troubleshooting guide may be helpful in solving any problems that may arise. For more information, see also the Frequently Asked Questions page at our Technical Support Center: www.qiagen.com/FAQ/FAQList.aspx. The scientists in QIAGEN Technical Services are always happy to answer any questions you may have about either the information and protocols in this handbook or sample and assay technologies (for contact information, see back cover or visit www.qiagen.com).

Comments and suggestions

No product, or product detected late in PCR

- | | |
|---|--|
| a) Annealing step (FRET probes and Molecular Beacons) or annealing/extension step (dual-labeled probes) too short | Always use the annealing time or annealing/extension time specified in the protocol. In some cases, increasing the time in steps of 10 s can improve results, especially with the LightCycler 1.x and 2.0. |
| b) Extension time too short (FRET probes and Molecular Beacons) | Always use the extension time specified in the protocol. In some cases, increasing the time in steps of 10 s can improve results, especially with the LightCycler 1.x and 2.0. |
| c) Wrong detection step | Ensure that fluorescence detection takes place during the annealing step when using FRET probes and Molecular Beacons, or during the combined annealing/extension step when using dual-labeled probes. |
| d) Pipetting error or missing reagent | Check the concentrations and storage conditions of the reagents, including primers, probe, and template RNA. * Repeat the RT-PCR. |
| e) HotStarTaq DNA Polymerase not activated | Ensure that the cycling program included the HotStarTaq DNA Polymerase activation step (15 min at 95°C) as described in the protocols. |

* For details, refer to "Guidelines for real-time PCR" at www.qiagen.com/resources/info.

Comments and suggestions

- | | |
|---|---|
| f) HotStarTaq DNA Polymerase activated too early | Check the cycling program. Ensure that the reverse-transcription reaction is complete before activating HotStarTaq DNA Polymerase.
LightCycler 1.x and 2.0: 20 min at 50°C
All other cyclers: 30 min at 50°C |
| g) Incorrect temperature for RT reaction | We recommend performing the RT reaction at 50°C. However, if this temperature does not yield satisfactory results, the temperature can be adjusted between 48°C and 55°C. |
| h) Incorrect amount of QuantiTect RT Mix | Use the correct amount of QuantiTect RT Mix.
LightCycler 480: 0.1 µl RT Mix per reaction
LightCycler 1.x and 2.0: 0.2 µl RT Mix per reaction
SmartCycler and Applied Biosystems 7500 Fast System: 0.25 µl RT Mix per reaction
All other cyclers: 0.5 µl RT Mix per reaction |
| i) Incorrect ratio of QuantiTect RT Mix to QuantiTect Probe RT-PCR Master Mix | If not using the standard reaction volumes, ensure that the volume of QuantiTect RT Mix is changed proportionately so that the ratio of QuantiTect RT Mix to QuantiTect Probe RT-PCR Master Mix remains the same. |
| j) RT-PCR product too long | For optimal results, RT-PCR products should be between 60 and 150 bp. RT-PCR products should not exceed 300 bp. |
| k) Primer design not optimal | Check for RT-PCR products by gel electrophoresis. If no specific RT-PCR products are detected, review the primer design guidelines.* |

* For details, refer to "Guidelines for real-time PCR" at www.qiagen.com/resources/info.

Comments and suggestions

- | | | |
|----|--|---|
| l) | Primer concentration not optimal | <p>Use optimal primer concentrations.</p> <p>SmartCycler and LightCycler 1.x and 2.0:
1 μM each primer.</p> <p>All other cyclers: 0.4 μM each primer.</p> <p>In some cases, increasing the primer concentration up to 2 μM can improve results.</p> <p>Check the concentrations of primers by spectrophotometry.*</p> |
| m) | Mg ²⁺ concentration not optimal | <p>Always start with the Mg²⁺ concentration provided in 2x QuantiTect Probe RT-PCR Master Mix (4 mM final concentration). For a few targets, an increase up to 6 mM Mg²⁺ may be helpful. Perform the titration in 0.5 mM steps.</p> |
| n) | Problems with starting template | <p>Check the concentration, storage conditions, and quality of the starting template RNA.*</p> <p>If necessary, make new serial dilutions of template RNA from the stock solutions. Repeat the RT-PCR using the new dilutions.</p> |
| o) | Insufficient amount of starting template | <p>Increase the amount of template, if possible. Ensure that sufficient copies of the target RNA are present in your sample.</p> |
| p) | Insufficient number of cycles | <p>Increase the number of cycles.</p> |
| q) | Probe design not optimal | <p>If the amplification reaction was successful, there may be a problem with the probe. Review the probe design guidelines.*</p> <p>If using Molecular Beacons, visit www.molecular-beacons.org for details on probe design.</p> |
| r) | Annealing temperature too high | <p>Decrease annealing temperature in steps of 2°C.</p> |
| s) | Annealing temperature too low | <p>Increase annealing temperature in steps of 2°C.</p> |

* For details, refer to "Guidelines for real-time PCR" at www.qiagen.com/resources/info.

Comments and suggestions

- | | |
|--------------------------------|---|
| t) No detection activated | Check that fluorescence detection was activated in the cycling program. |
| u) Probe synthesis not optimal | Check the quality of dual-labeled probes or Molecular Beacons by incubation with DNase I. A correctly synthesized probe, containing both fluorophore and quencher, will show a significant increase in fluorescence after DNase I incubation. |
| v) Primers degraded | Check for possible degradation of primers on a denaturing polyacrylamide gel. |
| w) Transcript not expressed | Repeat the RT-PCR and include a positive control to make sure the absence of RT-PCR product was not due to problems with reverse transcription, amplification, and detection.* |
| x) Heat-labile UNG not used | When performing optional UNG pretreatment before starting RT-PCR, be sure to use heat-labile UNG. UNG from <i>E. coli</i> is stable at elevated temperatures and will destroy any cDNA synthesized during reverse transcription at 50°C. |

Real-time cyclers other than the LightCycler 1.x and 2.0:

- | | |
|--|--|
| y) Wrong detection channel/filter chosen | Ensure that the correct detection channel is activated or the correct filter set is chosen for the reporter dye. |
|--|--|

LightCycler 1.x. and 2.0 only:

- | | |
|-----------------------------------|--|
| z) Wrong detection channel chosen | Ensure that the correct detection channel is chosen (e.g., F1 for FAM labeled TaqMan probes or Molecular Beacons; F2 for LC-Red 640 labeled FRET probes; and F3 for LC-Red 705 labeled FRET probes). |
|-----------------------------------|--|

* For details, refer to "Guidelines for real-time PCR" at www.qiagen.com/resources/info.

No linearity in ratio of C_T value/crossing point to log of the template amount

- | | | |
|----|---------------------------------------|---|
| a) | Template amount too high | Do not exceed maximum recommended amounts of template.

LightCycler 1.x and 2.0: Do not use more than 1 µg template.

All other cyclers: Do not use more than 500 ng template. |
| b) | Template amount too low | Increase template amount, if possible. |
| c) | Incorrect amount of QuantiTect RT Mix | Use the correct amount of QuantiTect RT Mix.

LightCycler 480: 0.1 µl RT Mix per reaction
LightCycler 1.x and 2.0: 0.2 µl RT Mix per reaction
SmartCycler and Applied Biosystems 7500 Fast System: 0.25 µl RT Mix per reaction
All other cyclers: 0.5 µl RT Mix per reaction |

High fluorescence in “No Template” control

- | | | |
|----|-------------------------------------|---|
| a) | Contamination of reagents | Discard all the components of the assay (e.g., master mix, primers, and probes). Repeat the assay using new components. |
| b) | Contamination during reaction setup | Take appropriate precautions during reaction setup, such as using aerosol-barrier pipet tips.

Use heat-labile uracil-N-glycosylase to prevent carryover from previous reactions. |

High fluorescence in “No Reverse Transcription” control

- | | |
|--|--|
| Contamination of RNA sample with genomic DNA | Design primers and/or probes that span exon–exon boundaries, so that only cDNA targets can be amplified and detected.

Alternatively, treat the RNA sample with DNase to digest the contaminating genomic DNA. |
|--|--|

Varying fluorescence intensity

- | | | |
|----|--|---|
| a) | Contamination of real-time cyclers | Decontaminate the real-time cyclers according to the manufacturer's instructions. |
| b) | Real-time cyclers no longer calibrated | Recalibrate the real-time cyclers according to the manufacturer's instructions. |

All cyclers systems:

- | | | |
|----|-------------------------------------|--|
| c) | Wavy curve at high template amounts | In the analysis settings, reduce the number of cycles used for background calculation (if your real-time cycler allows you to do so) or reduce the amount of template. |
|----|-------------------------------------|--|

ABI PRISM® 7000 only:

- | | | |
|----|---|--|
| d) | Uneven curves or high standard deviations | Do not use reaction volumes smaller than 25 µl and always use optical adhesive covers to seal plates. In some cases, increasing the reaction volume to 50 µl may improve results.

The halogen bulb is too old. Replace the bulb every 3 months (or after a maximum of 2000 live hours). |
|----|---|--|

LightCycler 1.x and 2.0 only:

- | | | |
|----|--------------------------------------|--|
| e) | RT-PCR mix not in capillary tip | Centrifuge the capillary to bring the RT-PCR mix into the capillary tip. |
| f) | Capillary not pushed down completely | Ensure that the capillary is completely pushed down in the LightCycler carousel. |
| g) | Wrong detection channel | Make sure that the correct channel is chosen. |

Ordering Information

Product	Contents	Cat. no.
QuantiTect Probe RT-PCR Kit (200)	For 200 x 50 µl reactions: 3 x 1.7 ml 2x Master Mix, 100 µl RT Mix, 2 x 2 ml RNase-Free Water	204443
QuantiTect Probe RT-PCR Kit (1000)	For 1000 x 50 µl reactions: 25 ml 2x Master Mix, 0.5 ml RT Mix, 20 ml RNase-Free Water	204445
Related products		
QuantiTect Probe PCR Kit — for quantitative, real-time PCR and two-step RT-PCR using sequence-specific probes		
QuantiTect Probe PCR Kit (40)	For 40 x 50 µl reactions: 1 ml 2x Master Mix, 2 ml RNase-Free Water	204341
QuantiTect Probe PCR Kit (200)	For 200 x 50 µl reactions: 3 x 1.7 ml 2x Master Mix, 2 x 2 ml RNase-Free Water	204343
QuantiTect Probe PCR Kit (1000)	For 1000 x 50 µl reactions: 25 ml 2x Master Mix, 20 ml RNase-Free Water	204345
QuantiTect Probe PCR +UNG Kit (200)	For 200 x 50 µl reactions: 3 x 1.7 ml 2x Master Mix, 100 µl UNG Solution, 2 x 2 ml RNase-Free Water	204363

For up-to-date licensing information and product-specific disclaimers, see the respective QIAGEN kit handbook or user manual. QIAGEN kit handbooks and user manuals are available at www.qiagen.com or can be requested from QIAGEN Technical Services or your local distributor.

QIAGEN offers a wide range of products for DNA and RNA purification and real-time PCR analysis — to find the right products for your needs, visit www.qiagen.com/ProductFinder.

Trademarks: QIAGEN®, HotStarTaq®, Omniscript®, QuantiTect®, Rotor-Gene®, Sensiscript® (QIAGEN Group); Mx3000P®, Mx3005P®, Mx4000® (Agilent Technologies); SmartCycler® (Cepheid); ABI PRISM®, Applied Biosystems®, FAM™, ROX™ (Life Technologies Corporation); LC®, LightCycler®, TaqMan® (Roche Group). Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are not to be considered unprotected by law.

For applicable countries:

NOTICE TO PURCHASER: LIMITED LICENSE

Use of this product (QuantiTect Probe RT-PCR Kit) is covered by one or more of the following US patents and corresponding patent claims outside the US: 6,127,155, 5,677,152 (claims 1 to 23 only), 5,773,258 (claims 1 and 6 only), and claims outside the US corresponding to expired US Patent No. 5,079,352. The purchase of this product includes a limited, non-transferable immunity from suit under the foregoing patent claims for using only this amount of product for the purchaser's own internal research. No right under any other patent claim and no right to perform commercial services of any kind, including without limitation reporting the results of purchaser's activities for a fee or other commercial consideration, is conveyed expressly, by implication, or by estoppel. This product is for research use only. Diagnostic uses under Roche patents require a separate license from Roche. Further information on purchasing licenses may be obtained by contacting the Director of Licensing, Applied Biosystems, 850 Lincoln Centre Drive, Foster City, California 94404, USA.

NOTICE TO PURCHASER: LIMITED LICENSE.

The use of this product (QuantiTect Probe RT-PCR Kit) is covered by at least one claim of U.S. Patent No. 7,687,247 owned by Life Technologies Corporation. The purchase of this product conveys to the buyer the non-transferable right to use the purchased amount of the product and components of the product in research conducted by the buyer (whether the buyer is an academic or for-profit entity). The buyer cannot sell or otherwise transfer (a) this product, (b) its components, or (c) materials made by the employment of this product or its components to a third party or otherwise use this product or its components or materials made by the employment of this product or its components for Commercial Purposes. Commercial Purposes means any activity for which a party receives or is due to receive consideration and may include, but is not limited to: (1) use of the product or its components in manufacturing; (2) use of the product or its components to provide a service, information, or data; (3) use of the product or its components for therapeutic, diagnostic or prophylactic purposes; or (4) resale of the product or its components, whether or not such product or its components are resold for use in research. The buyer cannot use this product or its components or materials made using this product or its components for therapeutic, diagnostic or prophylactic purposes. Further information on purchasing licenses under the above patents may be obtained by contacting the Licensing Department, Life Technologies Corporation, 5791 Van Allen Way, Carlsbad, CA 92008. Email: outlicensing@lifetech.com.

NOTICE TO PURCHASER: LIMITED LICENSE

The purchase of this product (QuantiTect Probe RT-PCR Kit) includes a limited, non-transferable right to use the purchased amount of the product to perform Applied Biosystem's patented Passive Reference Method for the purchaser's own internal research. No right under any other patent claim and no right to perform commercial services of any kind, including without limitation reporting the results of purchaser's activities for a fee or other commercial consideration, is conveyed expressly, by implication, or by estoppel. This product is for research use only. For information on obtaining additional rights, please contact outlicensing@lifetech.com or Out Licensing, Life Technologies, 5791 Van Allen Way, Carlsbad, California 92008.

Limited License Agreement

Use of this product signifies the agreement of any purchaser or user of the QuantiTect Probe RT-PCR Kit to the following terms:

1. The QuantiTect Probe RT-PCR Kit may be used solely in accordance with the *QuantiTect Probe RT-PCR Handbook* and for use with components contained in the Kit only. QIAGEN grants no license under any of its intellectual property to use or incorporate the enclosed components of this Kit with any components not included within this Kit except as described in the *QuantiTect Probe RT-PCR Handbook* and additional protocols available at www.qiagen.com.
2. Other than expressly stated licenses, QIAGEN makes no warranty that this Kit and/or its use(s) do not infringe the rights of third-parties.
3. This Kit and its components are licensed for one-time use and may not be reused, refurbished, or resold.
4. QIAGEN specifically disclaims any other licenses, expressed or implied other than those expressly stated.
5. The purchaser and user of the Kit agree not to take or permit anyone else to take any steps that could lead to or facilitate any acts prohibited above. QIAGEN may enforce the prohibitions of this Limited License Agreement in any Court, and shall recover all its investigative and Court costs, including attorney fees, in any action to enforce this Limited License Agreement or any of its intellectual property rights relating to the Kit and/or its components.

For updated license terms, see www.qiagen.com.

© 2002–2011 QIAGEN, all rights reserved.

www.qiagen.com

Australia = Orders 1-800-243-800 = Fax 03-9840-9888 = Technical 1-800-243-066

Austria = Orders 0800-28-10-10 = Fax 0800/28-10-19 = Technical 0800-28-10-11

Belgium = Orders 0800-79612 = Fax 0800-79611 = Technical 0800-79556

Brazil = Orders 0800-557779 = Fax 55-11-5079-4001 = Technical 0800-557779

Canada = Orders 800-572-9613 = Fax 800-713-5951 = Technical 800-DNA-PREP (800-362-7737)

China = Orders 86-21-3865-3865 = Fax 86-21-3865-3965 = Technical 800-988-0325

Denmark = Orders 80-885945 = Fax 80-885944 = Technical 80-885942

Finland = Orders 0800-914416 = Fax 0800-914415 = Technical 0800-914413

France = Orders 01-60-920-926 = Fax 01-60-920-925 = Technical 01-60-920-930 = Offers 01-60-920-928

Germany = Orders 02103-29-12000 = Fax 02103-29-22000 = Technical 02103-29-12400

Hong Kong = Orders 800 933 965 = Fax 800 930 439 = Technical 800 930 425

Ireland = Orders 1800 555 049 = Fax 1800 555 048 = Technical 1800 555 061

Italy = Orders 800-789-544 = Fax 02-334304-826 = Technical 800-787980

Japan = Telephone 03-6890-7300 = Fax 03-5547-0818 = Technical 03-6890-7300

Korea (South) = Orders 080-000-7146 = Fax 02-2626-5703 = Technical 080-000-7145

Luxembourg = Orders 8002-2076 = Fax 8002-2073 = Technical 8002-2067

Mexico = Orders 01-800-7742-639 = Fax 01-800-1122-330 = Technical 01-800-7742-436

The Netherlands = Orders 0800-0229592 = Fax 0800-0229593 = Technical 0800-0229602

Norway = Orders 800-18859 = Fax 800-18817 = Technical 800-18712

Singapore = Orders 1800-742-4362 = Fax 65-6854-8184 = Technical 1800-742-4368

Spain = Orders 91-630-7050 = Fax 91-630-5145 = Technical 91-630-7050

Sweden = Orders 020-790282 = Fax 020-790582 = Technical 020-798328

Switzerland = Orders 055-254-22-11 = Fax 055-254-22-13 = Technical 055-254-22-12

UK = Orders 01293-422-911 = Fax 01293-422-922 = Technical 01293-422-999

USA = Orders 800-426-8157 = Fax 800-718-2056 = Technical 800-DNA-PREP (800-362-7737)

